
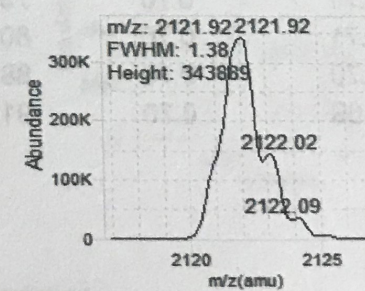
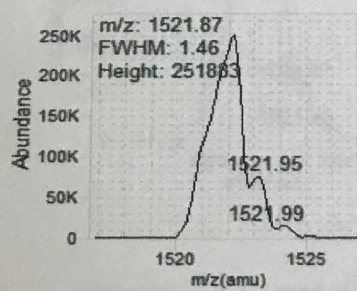
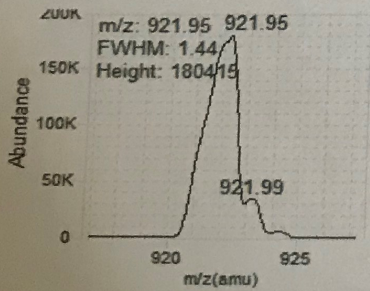
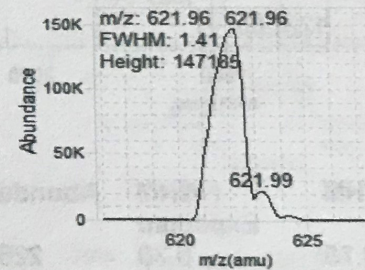
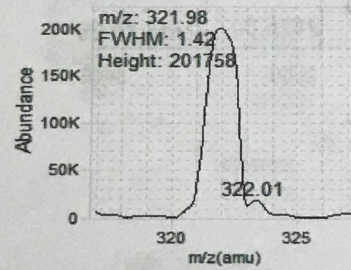


m/z	m/z Expected	FWHM	FWHM Expected	Abundance
118.02	118.09	1.21	1.20	349700
322.00	322.05	1.42	1.20	244611
621.97	622.03	1.39	1.20	176631
921.88	922.01	1.40	1.20	170158
1521.83	1521.97	1.34	1.20	188118
2121.85	2121.93	1.36	1.20	173695

Analyzer: MS2

Polarity: Positive

Width: Wide

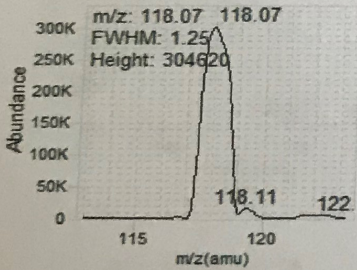

m/z	m/z Expected	FWHM	FWHM Expected	Abundance
118.07	118.09	1.25	1.20	304620
321.98	322.05	1.42	1.20	201758
621.96	622.03	1.41	1.20	147185
921.95	922.01	1.44	1.20	180415
1521.87	1521.97	1.46	1.20	251882
2121.92	2121.93	1.38	1.20	343889